


REVISONS				BILL OF MATERIALS						
REV	DESCRIPTION	DATE	DRAWN	APPROVED	ITEM	DESCRIPTION	QTY.	PART NO.	VENDOR	REV.
A	ITEM 1 WAS GRAY	06/11/01	T. MILLER(RFP)	T. MILLER(RFP)	1	CLEAR MALE HOSPITAL PLUG (NEMA 5-15P)	1	UC-018		
B	ITEM 3 WAS EC220	09/04/01	C. PRUITT	H. MAYER		NICKEL PLATED U-SHAPED GROUND PIN		98478		
C	PLACED DIM ON NEW TEMPLATE. ITEM 3 ADD. GEN 38478 & INCORPORATE NOTE 2. ITEM 3 ADD. GEN 38478 TO TOP OF OVERALL. METRIC DIM WAS 3.0MMETERS 2.25" DIA. COMBINED NOTES 2, 3, 4, 5 INTO NOTES 2&3 & ADD 500 PACKAGED. WORKED. 50/100 LB. TO DIM DETAIL. ADD 50/100 LB. TO DIM DETAIL. ADD 50/100 LB. TO DIM DETAIL. ADD 50/100 LB. TO DIM DETAIL.	02/18/04	C. PRUITT	N. WALDRON	2	GRAY (GY-56) SJT 18/3 105°C VW-1 NA BC 5 STRANDING (41x34)	*	N/A	N/A	
D	ADD 2 TWIST TIES TO COIL	03/04/04	C. PRUITT	N. WALDRON	3	GRAY (GY-56) FEMALE CONNECTOR (IEC 60320/C13) PHOS. BRONZE CONTACTS	1	UC-005		
E	ADD VW-1 TO ITEM 2	07/14/04	C. PRUITT	H. MAYER				98741		
F	CORRECTED CSA FILE NO FROM 1L7784G. ADDED PLUG MARK & RPHS NOTES.	06/15/06	A. RICE	L. ODEN						
G	CORRECTED CSA LABEL. REMOVED APPROVAL LOGOS, UL/CUL LABEL, & PLUG MARK FROM NOTES. ADDED APPROVALS. NOTE	12/20/07	A. RICE	L. ODEN	4	UL CORD SET 10A/125V RATING TAG	1	UL-0097		

NOTES:

1. ELECTRICAL RATING: 10A/125V
2. APPROVALS: UL/CUL/CSA
3. UL/CUL FILE NO E147232, MEETS STANDARD UL 817
4. CSA FILE NO LL77839, MEETS STANDARD CSA C22.2 NO. 21.
5. RoHS COMPLIANT.

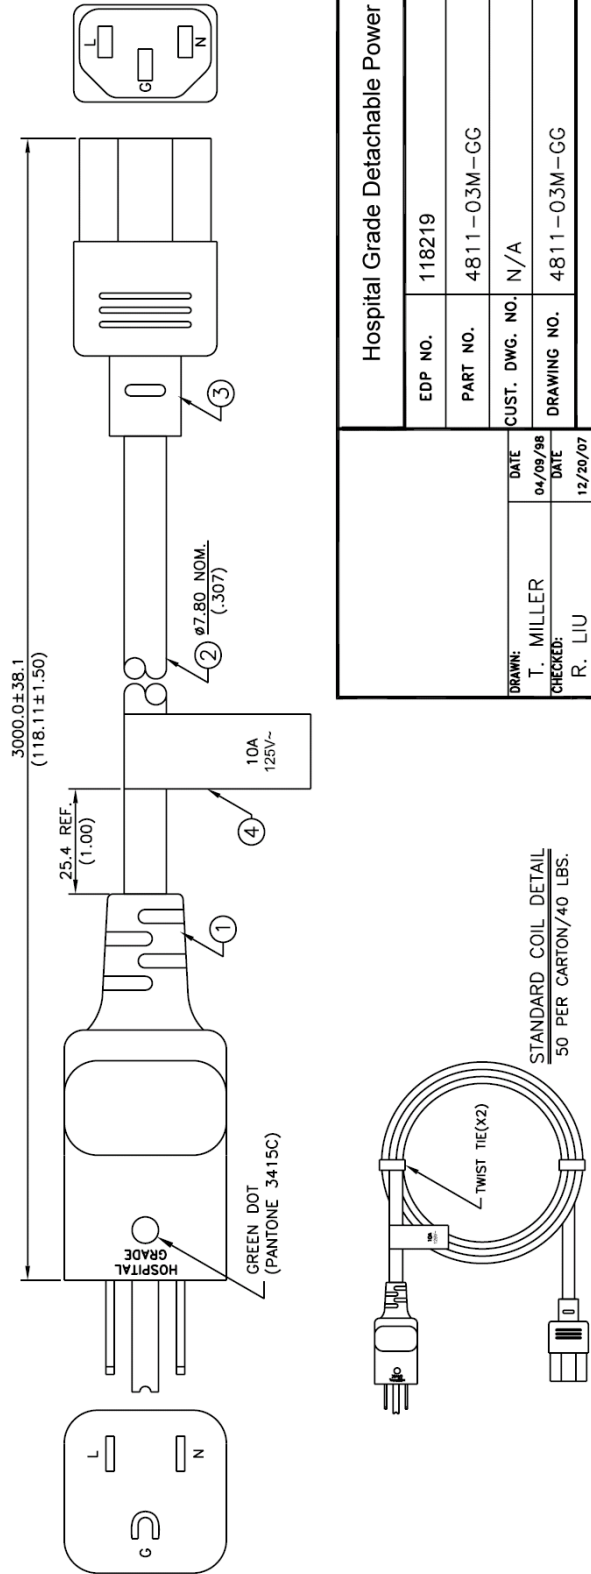

DRAWN:		DATE
T. MILLER		04/09/98
CHECKED:		DATE
R. LIU		12/20/07
APPROVAL:		DATE
L. ODEN		12/20/07

Hospital Grade Detachable Power Cord		
EDP NO.	118219	REV.
PART NO.	4811-03M-GG	REV.
CUST. DWG. NO.	N/A	REV.
DRAWING NO.	4811-03M-GG	REV.

STANDARD COIL DETAIL
50 PER CARTON/40 LBS.